


Hamse M product 2 analogue catalyst
P31CPD CDC13 /opt/data Adv_Exp 29

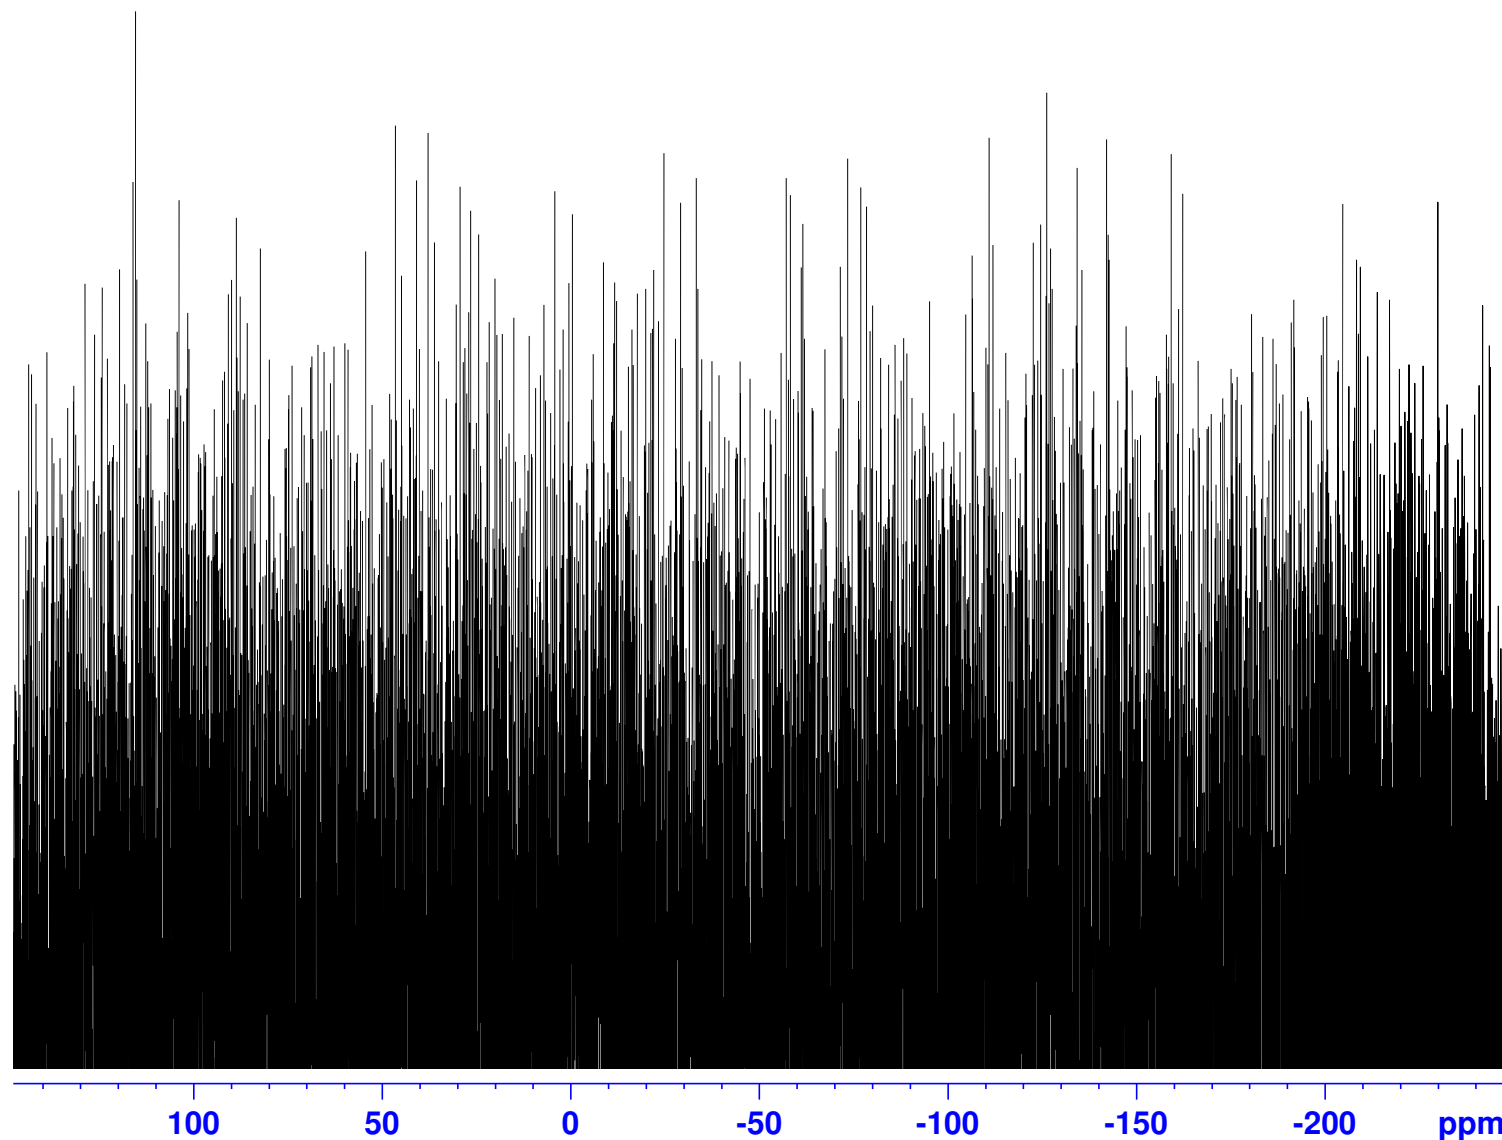

Current Data Parameters
NAME X_20190221
EXPNO 99
PROCNO 1

F2 - Acquisition Parameters
Date_ 20190221
Time 14.58 h
INSTRUM spect
PROBHD Z824801_0046 (
PULPROG zgpg30
TD 65536
SOLVENT CDC13
NS 16
DS 4
SWH 64102.562 Hz
FIDRES 1.956255 Hz
AQ 0.5111808 sec
RG 200.25
DW 7.800 usec
DE 6.50 usec
TE 300.0 K
D1 2.00000000 sec
D11 0.03000000 sec
TD0 1
SFO1 162.0079729 MHz
NUC1 31P
P0 2.67 usec
P1 8.00 usec
PLW1 36.45100021 W
SFO2 400.2316009 MHz
NUC2 1H
CPDPRG[2] waltz16
PCPD2 90.00 usec
PLW2 20.00000000 W
PLW12 0.23714000 W
PLW13 0.11928000 W

F2 - Processing parameters
SI 32768
SF 162.0160737 MHz
WDW EM
SSB 0
LB 1.00 Hz
GB 0
PC 1.40

1.40
1.48
0.91
1.25
0.50
0.43
0.62
2.48
0.90
1.43
3.54
1.21
0.96
0.07
2.18
1.62
1.73
2.16
2.09
0.05
1.00
2.57
0.30
0.60
1.72
1.79
0.93
1.03
0.31
0.19
1.82
0.26
1.83
0.29
1.26
2.03
0.11
1.35
1.03
1.30
0.03
1.57
1.27
1.11
1.50