


mw1

F19.qm CDC13 /opt/data Adv Exp 6

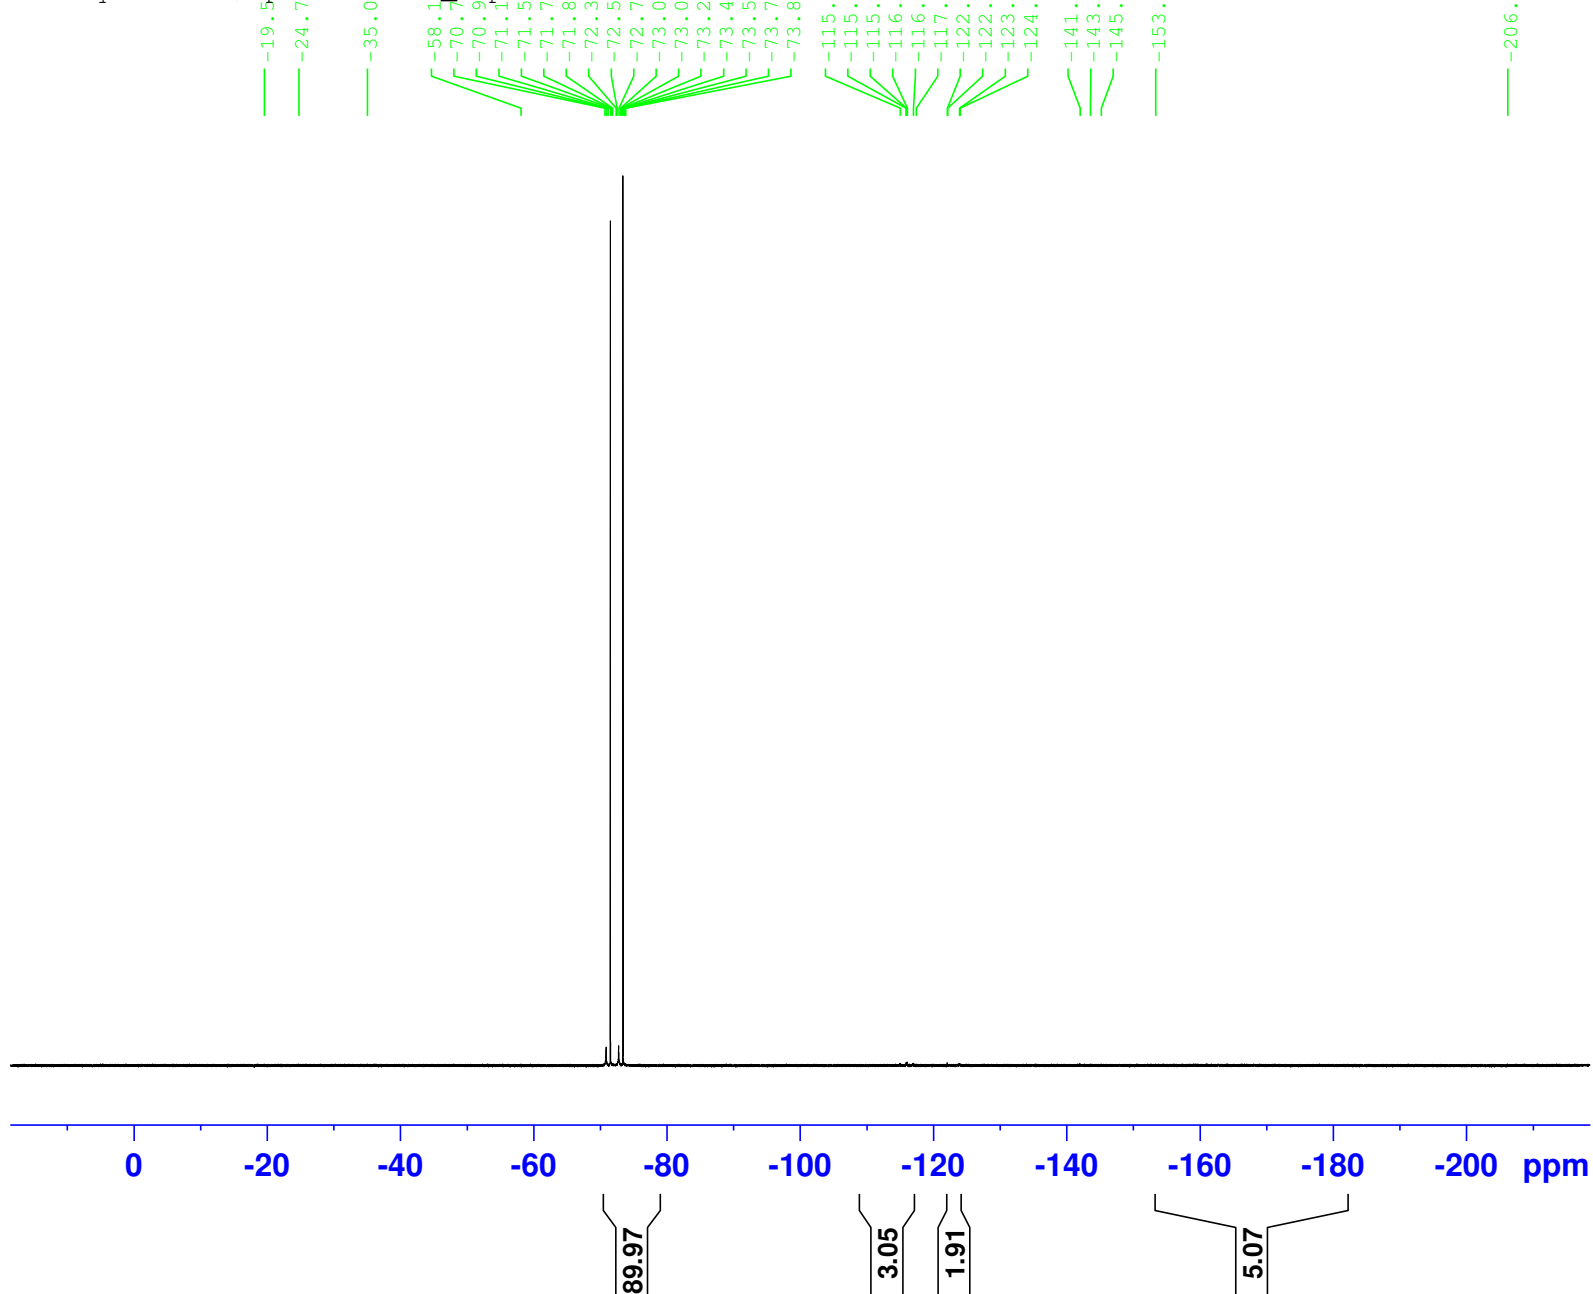

Current Data Parameters
NAME X_210923
EXPNO 60
PROCNO 1

F2 - Acquisition Parameters
Date_ 20210923
Time 19.23 h
INSTRUM aviii400
PROBHD z108618_0305 (
PULPROG zgflqn180.b
TD 267848
SOLVENT CDC13
NS 16
DS 2
SWH 89285.711 Hz
FIDRES 0.666689 Hz
AQ 1.4999489 sec
RG 912
DW 5.600 usec
DE 6.88 usec
TE 300.0 K
D1 2.00000000 sec
L0 1
TD0 1
SFO1 376.5265758 MHz
NUC1 19F
P1 11.70 usec
P26 2000.00 usec
PLW0 0 W
PLW1 28.84000015 W
SPNAM[8] Crp180,2,20.1
SPOAL8 0
SPOFFS8 0 Hz
SPW8 4.52400017 W

F2 - Processing parameters
SI 262144
SF 376.5642320 MHz
WDW EM
SSB 0
LB 1.00 Hz
GB 0
PC 1.00