
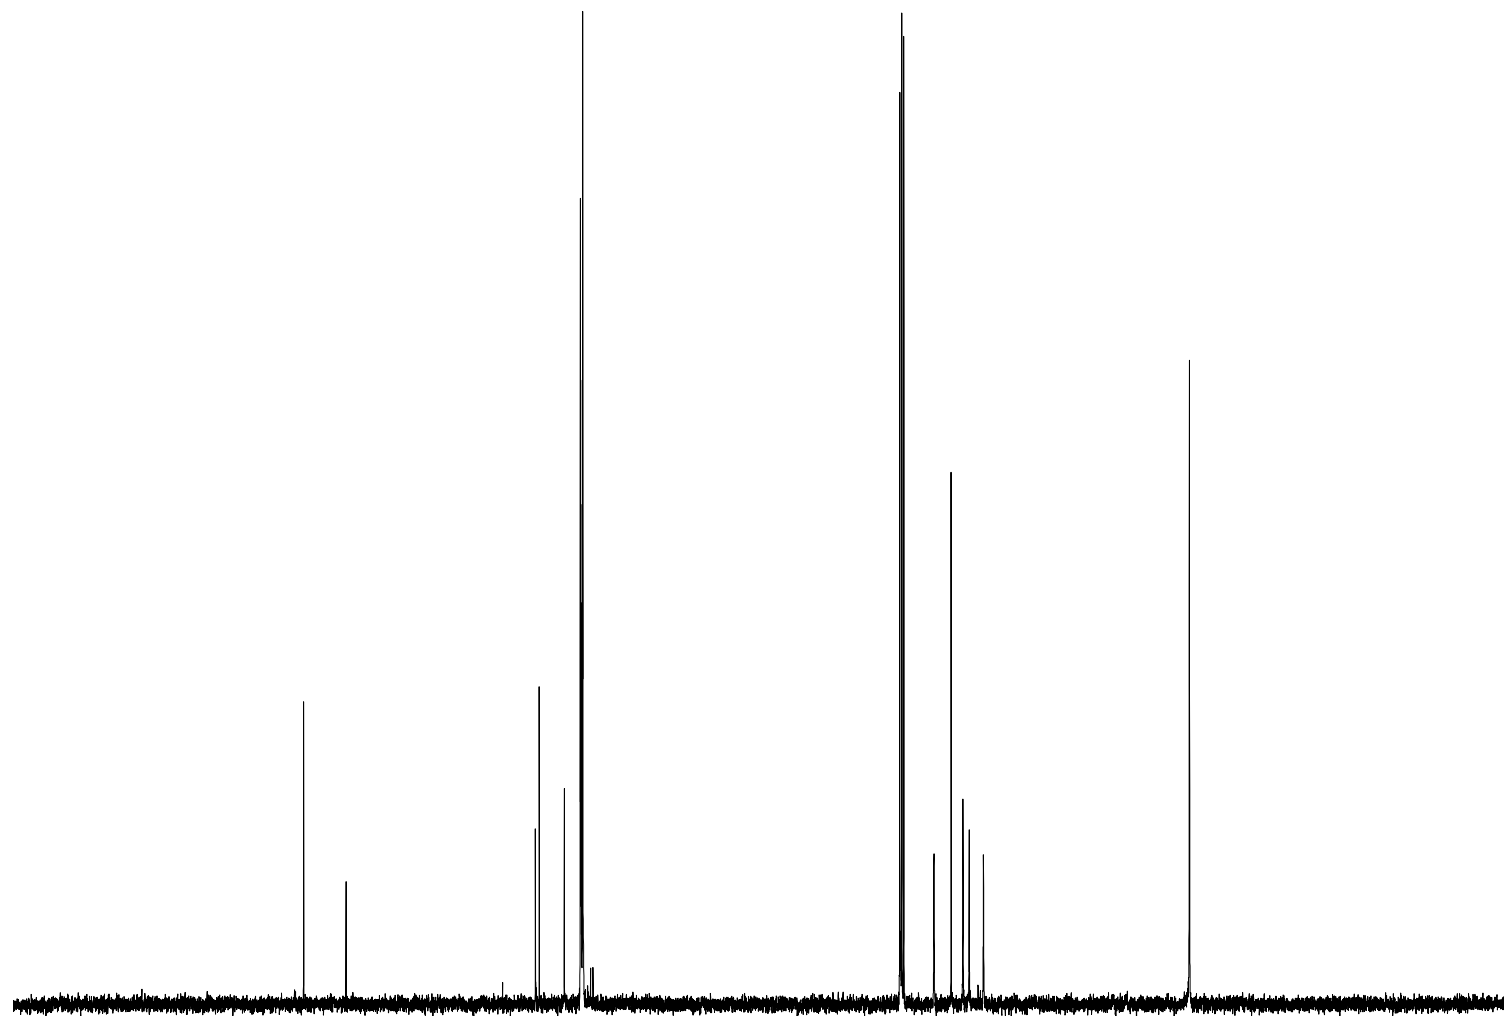


AF

C13CPD256 CDC13 /opt/data Adv\_Exp\_48

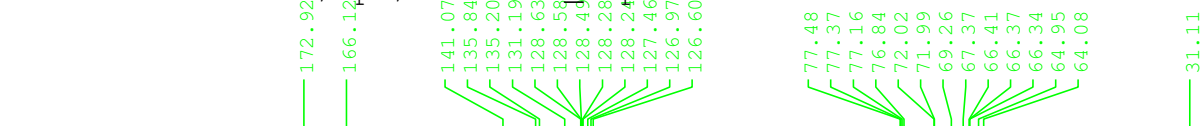

Current Data Parameters  
 NAME X\_240213  
 EXPNO 91  
 PROCNO 1

F2 - Acquisition Parameters  
 Date\_ 20240214  
 Time 12.39 h  
 INSTRUM aviii400  
 PROBHD Z108618\_0305 (  
 PULPROG zgpg30  
 TD 65536  
 SOLVENT CDC13  
 NS 256  
 DS 4  
 SWH 24038.461 Hz  
 FIDRES 0.733596 Hz  
 AQ 1.3631488 sec  
 RG 2050  
 DW 20.800 usec  
 DE 6.50 usec  
 TE 300.0 K  
 D1 2.00000000 sec  
 D11 0.03000000 sec  
 TD0 1  
 SFO1 100.6404326 MHz  
 NUC1 13C  
 P0 3.27 usec  
 P1 9.80 usec  
 PLW1 50.11899948 W  
 SFO2 400.2016008 MHz  
 NUC2 1H  
 CPDPRG[2] waltz16  
 PCPD2 90.00 usec  
 PLW2 19.95299911 W  
 PLW12 0.36664000 W  
 PLW13 0.18442000 W

F2 - Processing parameters  
 SI 32768  
 SF 100.6303700 MHz  
 WDW EM  
 SSB 0  
 LB 1.00 Hz  
 GB 0  
 PC 1.40