


Propanal Std. + acetone
PROTON.qm CDCl₃ /opt/data Adv_Exp 5

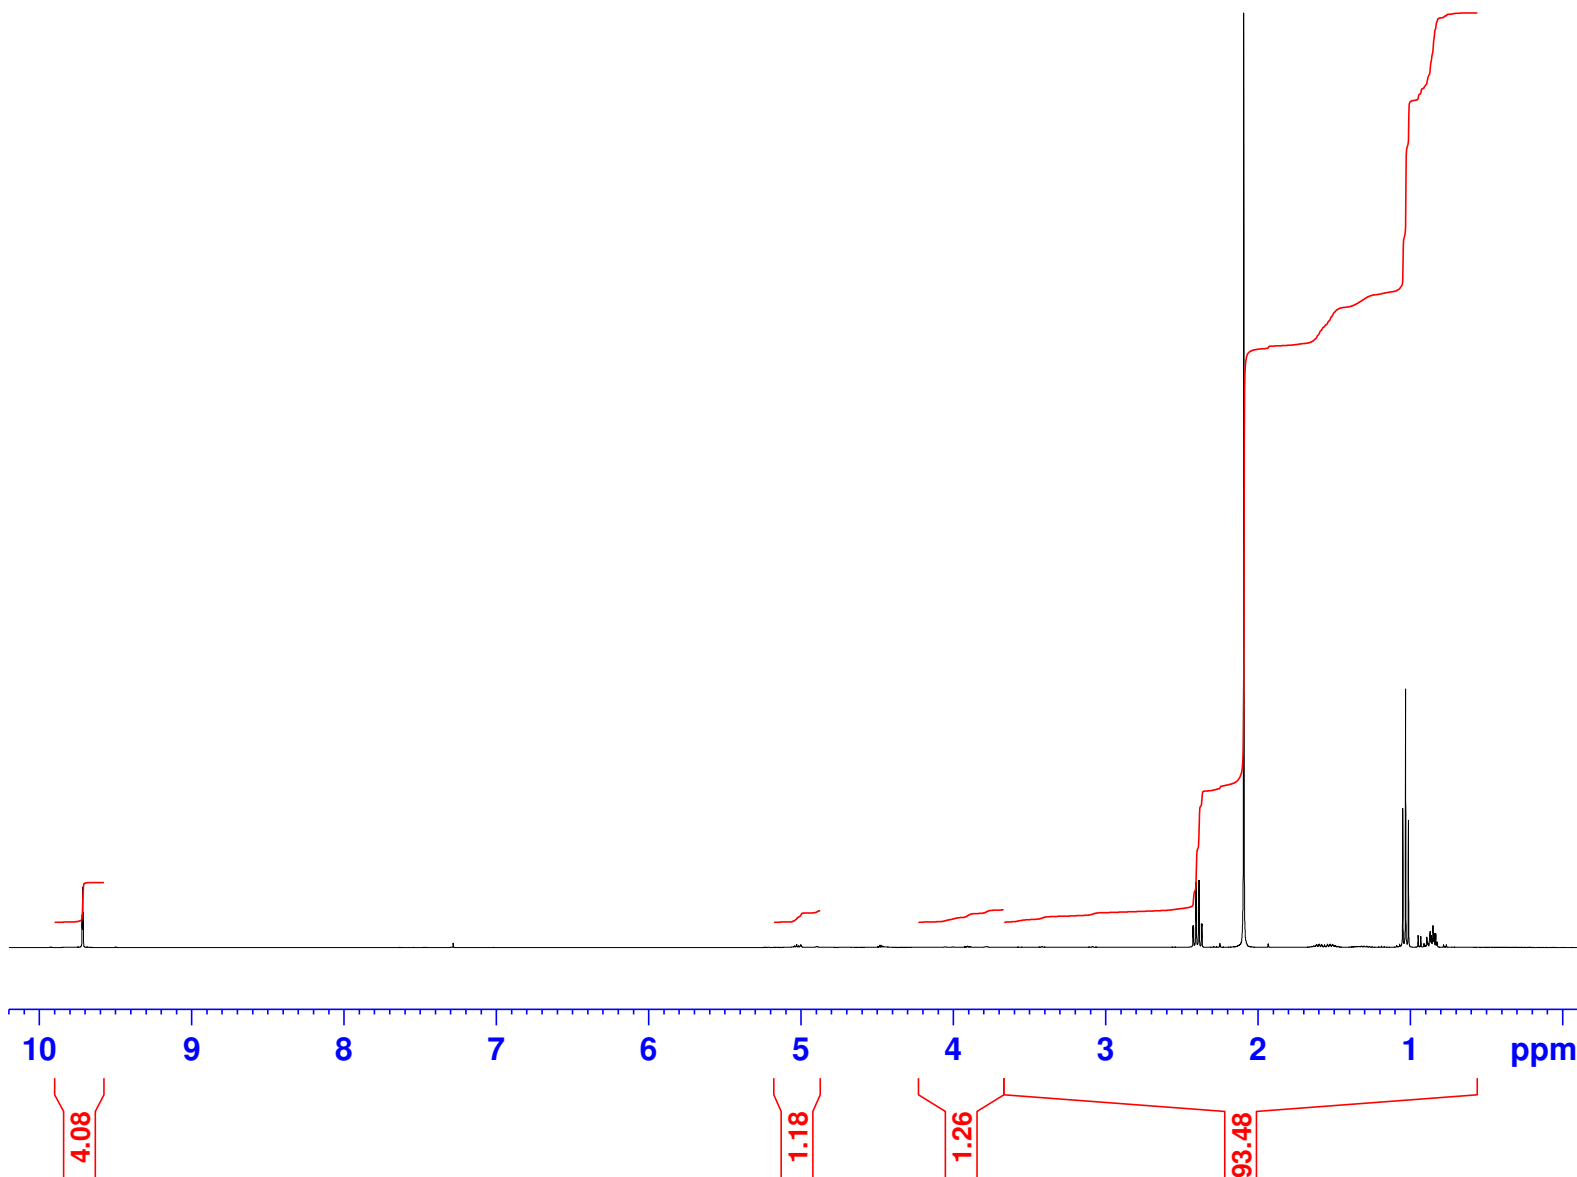

Current Data Parameters
NAME X_250411
EXPNO 41
PROCNO 1

F2 - Acquisition Parameters
Date_ 20250411
Time 16.01 h
INSTRUM aviii400
PROBHD z108618_0305 (
PULPROG zg30
TD 65536
SOLVENT CDCl₃
NS 16
DS 0
SWH 8223.685 Hz
FIDRES 0.250967 Hz
AQ 3.9845889 sec
RG 32
DW 60.800 usec
DE 15.65 usec
TE 300.0 K
D1 1.00000000 sec
TD0 1
SFO1 400.2024714 MHz
NUC1 1H
P0 6.50 usec
P1 19.50 usec
PLW1 19.95299911 W

F2 - Processing parameters
SI 65536
SF 400.2000000 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00